


InertSearch™ for LC

Inertsil® Applications

Analysis of Glutathione HPLC-ECD

Data No. LA956-0142

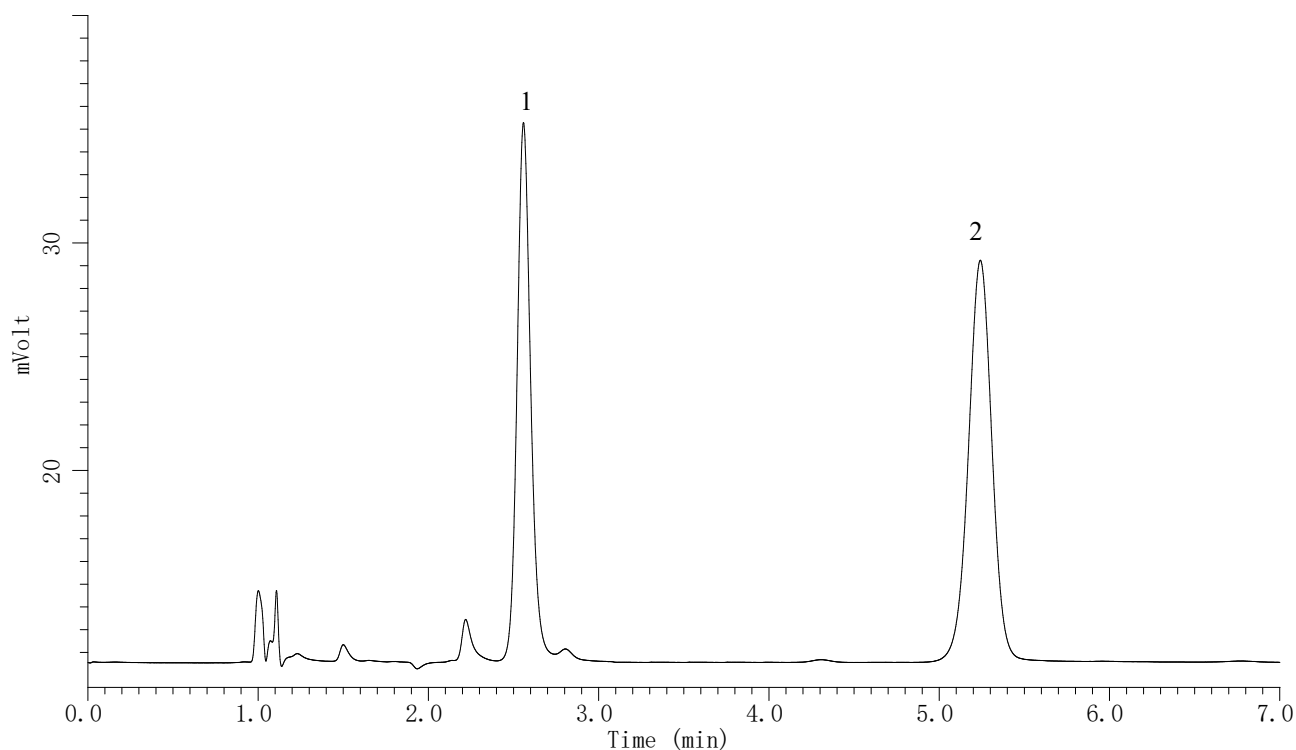

Conditions

System : LC800 HPLC system
Column : InertSustain C18 HP (3 μ m, 150 x 3.0 mm I.D.)
Column Cat. No. : 5020-14425
Eluent : 50 mM NaH₂PO₄ (pH 2.2, H₃PO₄)
Flow Rate : 0.6 mL/min
Col. Temp. : 40 °C
Detection : ECD 1200 mV vs Ag/AgCl (ED723 EC Detector, Diamond)
Injection Vol. : 5 μ L
Sample : Standard

Analyte:


1. Glutathione (GSH) (1 μ g/mL)
2. Glutathione Disulfide (GSSG) (1 μ g/mL)

InertSearch™ for LC

Inertsil® Applications

Analysis of Glutathione HPLC-ECD

Data No. LA956-0142

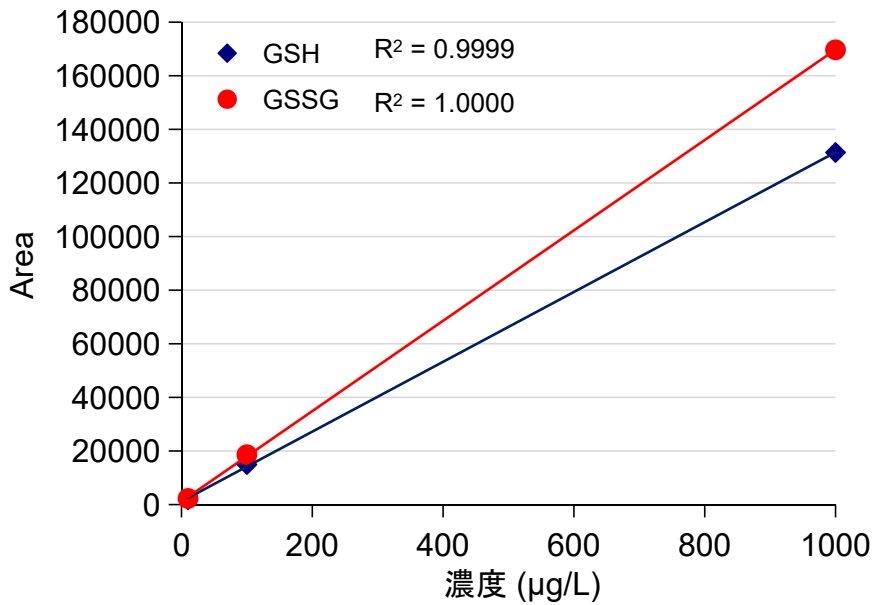

【検量線】